


Specifications

MGAI

Amplifier system

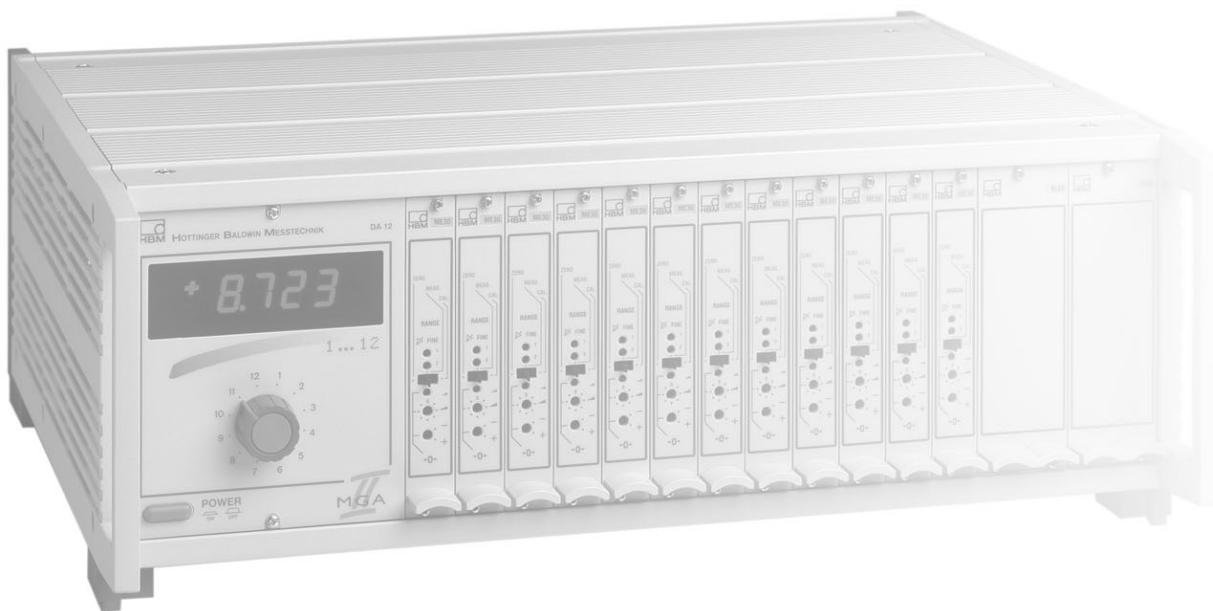


Technical Data, system unit


Mains power supply	V AC	115 V/230 V -25+15 %
Nominal input voltage	A	2.2/1.3
Max. nominal input current	A	< 20
Starting current		
Max. power consumption	W	83
Nominal temperature range	°C	-10...+60
Service temperature range	°C	-20...+60
Storage temperature range	°C	-25...+70
Protection Class		Desktop housing IP20 19" module frame IP20

Housing dimensions (WxHxD in mm; 1 mm= 0.0397 inches)


TG 005 desktop housing
(255x171x367)

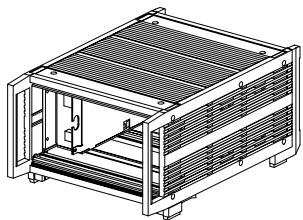


TG 007 desktop housing (458x171x367)

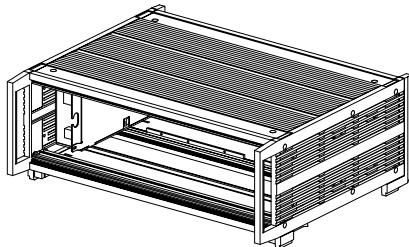

TG011 desktop housing (173x171x367)



ER 007 19" module frame (483x132.5x367)

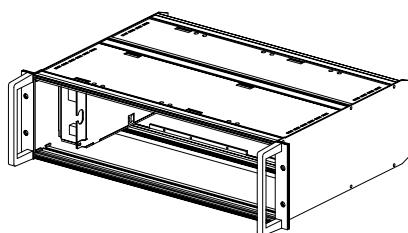

Desktop housing	Module frame	Max. number of channels	Supply voltage
TG005	-	6	230 V (115 V)~
TG007	-	12	230 V (115 V)~
TG011	-	2	230 V (115 V)~
-	ER007	12	230 V (115 V)~

Technical Data, DA12 numeric display

Accuracy class		0.05	
Numeric indication range			
Nominal value	d		± 10,000
Peak value	d		± 19,999
Input			
Measurement channels			12
Differential input voltage for nominal display value	V		± 10.000
Differential input voltage, maximum value	V		± 19.999
Input resistance			
Permissible common-mode rejection against zero operating voltage	kΩ		> 100
Common-mode rejection	V		± 1
			> 50
Measurement display	mm		
Polarity indication			14
Decimal-point indication (can be enabled/disabled with St21)			Seven-segment display automatic 10,000; fixed
Overload detector	V		> ± 10
Measurement time /conversion time)	s		0.4
Integration time	s		0.1
Linearity variance in the nominal range 10000d	d		± 1
Error of symmetry in the nominal range 10,000d	d		± 1
Effect of 10 K change in ambient temperature			
on zero point	%		0.005 of final value
on sensitivity	%		0.03

ME10 amplifier plug-in unit

Type	ME10			
Accuracy class	0.1			
Bridge supply voltage	V	2.5± 2 %	5± 2 %	10± 2 %
Attachable process-quantity transducer				
Strain-gauge transducer (full bridge)	Ω	60...4000	110...4000	220...4000
Maximum cable length	m		500	
			2	
Number of ranges				
Ranges, adjustable in 12 steps	mV/V	0.4...8	0.2...4	0.1...2
Continuous fine adjustment	%		35	
Factory setting: Range 1	mV/V		± 2	
Range 2	mV/V		± 0.2	
Calibration signal	mV/V		+ 1 ± 0.1 %	
Bridge balance range	mV/V		± 2	
Coarse balance, adjustable in 16 steps (polarity adjustable)	mV/V		± 2	
Fine balance, using screwdriver potentiometer	mV/V		± 0.08	
Measurement frequency range		Butterworth low pass 3rd order		Without low-pass
at -1 dB	Hz	0...2	0...500	0...10,000
at -3 dB	Hz	2.5	675	20,000
Phase delay time	ms	135	0.55	0.01
Rise time	ms	170	0.5	0.015
Overshoot at sudden change in signal	%	<10	<10	<0.1
Input (symmetrical)				
Input impedance	MΩ par. pF		>20 200	
Permitted common-mode voltage	V		± 6 V	
Common-mode rejection	dB	DC		0...500 Hz
		>130		100
Output (asymmetrical)				
Nominal voltage	V		± 10	
Permissible load resistance	kΩ		>5	
Internal resistance	Ω		<5	
Noise , at UB=5 V projected backwards to the input (peak-to-peak value)	µV/V	<0.1	<0.5	<2
Linearity variance relative to nominal voltage	%	<0.01		
Effect of temperature per 10 K in the nominal temperature range, relative to sensitivity	%	<0.1; typically 0.05		
to the zero point at the amplifier output				
in the range 2 mV/V at UB=5 V (4x350 Ω)	mV	<10, or		
in the range 0.2 mV/V at UB=5 V	mV	<100; also <0.05% of the bridge balance value		
Long-term drift over 48 hours (after 1h warm-up time)	µV/V	<0.1		

ME30 amplifier plug-in unit

Type	ME30		
Accuracy class	0.1		
Carrier frequency	Hz	$600 \pm 0.5\%$	
Bridge supply voltage	V	$2.5 \pm 2\%$	$5 \pm 2\%$
Attachable process-quantity transducer			
Strain-gauge transducer (full bridge)	Ω	60...4000	110...4000
Maximum cable length	m	500	
Number of ranges		2	
Ranges, adjustable in 12 steps	mV/V	0.4...8	0.2...4
Continuous fine adjustment	%	35	
Factory setting: Range 1	mV/V	± 2	
Range 2	mV/V	± 0.2	
Calibration signal	mV/V	$+1 \pm 0.1\%$	
Bridge balance range		± 2	
Coarse balance, adjustable in 16 steps (polarity adjustable)	mV/V	± 2	
Fine balance, using screwdriver potentiometer	mV/V	± 0.08	
Measurement frequency range		Butterworth low-pass 3rd order, switchable	
at -1 dB	Hz	0...2	0...60
at -3 dB	Hz	2.5	80
Phase delay time	ms	135	4.8
Rise time	ms	170	7
Overshoot at sudden change in signal	%	<10	
Residual carrier voltage	%	<0.1	<0.2; typically 0.1
Input (symmetrical)			
Input impedance	$M\Omega$ par. pF	>10 470	
Permitted common-mode voltage	V	$\pm 6\text{ V}$	
Common-mode rejection	dB	0...600 Hz: >50	
Output (asymmetrical)			
Nominal voltage	V	± 10	
Permissible load resistance	$k\Omega$	>5	
Internal resistance	W	<5	
Noise , projected backwards to the input	$\mu\text{V/V}$	<0.2 (peak-to-peak); typically 0.1	
Linearity variance relative to nominal voltage	%	<0.02; typically 0.01	
Effect of temperature per 10 K in the nominal temperature range relative to sensitivity	%	<0.1; typically 0.05	
to the zero point at the amplifier output			
in the range 2 mV/V at $U_B=5\text{ V}$ ($4 \times 350\text{ }\Omega$)	mV	<4, or	
in the range 0.2 mV/V at $U_B=5\text{ V}$	mV	<13; also <0.05 % of the bridge balance value	
Long-term drift over 48 hours (after 1 h warm-up time)	$\mu\text{V/V}$	<0.05	

ME50 amplifier plug-in unit


Type	ME50		
Accuracy class	0.1		
Carrier frequency	Hz	$4800 \pm 0.5\%$	
Bridge supply voltage	V	$1 \pm 3\%$	$2.5 \pm 2\%$
Attachable process-quantity transducer			
Inductive transducer (half bridge)	mH	2.5...20	
Maximum cable length	m	500	
Number of ranges		2	
Ranges, adjustable in 12 steps	mV/V	20...400	$8 \dots 160$
Continuous fine adjustment	%	35	
Factory setting: Range 1	mV/V	± 80	
Range 2	mV/V	± 8	
Calibration signal	mV/V	$+8 \pm 0.1\%$	
Bridge balance range		± 80	
Coarse balance, adjustable in 16 steps (polarity adjustable)	mV/V	± 80	
Fine balance, using screwdriver potentiometer	mV/V	± 3.2	
Measurement frequency range		Butterworth low-pass 3rd order, switchable	
at -1 dB	Hz	0...2	0...500
at -3 dB	Hz	2.5	675
Phase delay time	ms	135	0.55
Rise time	ms	170	0.5
Overshoot at sudden change in signal	%	<10	<10
Residual carrier voltage	%	<0.02	<0.2; typically 0.1
Input (symmetrical)			
Input impedance	MΩ par. pF	>0.2 100 $\pm 6\text{ V}$	
Permitted common-mode voltage	V	0...4800 Hz: > 50	
Common-mode rejection	dB		
Output (asymmetrical)			
Nominal voltage	V	± 10	
Permissible load resistance	kΩ	>5	
Internal resistance	Ω	<5	
Noise, projected backwards to the input	µV/V	500 Hz:<8 (peak-to-peak) 2 Hz:<0.08 (peak-to-peak)	500 Hz:<8 (peak-to-peak) 2 Hz:<0.08 (peak-to-peak)
Linearity variance	%	<0.05; typically 0.02	
relative to nominal voltage			
Effect of temperature per 10 K in the nominal temperature range relative			
to sensitivity	%	<0.15; typically 0.1	
to the zero point at the amplifier output	µV/V	<8; typically 4 also <0.05% of the bridge balance value	
Long-term drift over 48 hours (after 1 h warm-up time)	µV/V	<0.8	

ME50S6 amplifier plug-in unit


Type	ME50S6		
Accuracy class	0.1		
Carrier frequency	Hz	$4800 \pm 0.5\%$	
Bridge supply voltage	V	$1 \pm 2\%$	$5 \pm 2\%$
Attachable process-quantity transducer			
Strain-gauge transducer (full bridge)	Ω	60...4000	110...4000
Maximum cable length	m	500	
Number of ranges		2	
Ranges, adjustable in 12 steps	mV/V	1...20	$0.2 \dots 4$
Continuous fine adjustment	%	35	
factory setting: Range 1	mV/V	± 1	
Range 2	mV/V	± 0.2	
Calibration signal	mV/V	$+1 \pm 0.1\%$	
Bridge balance range		± 2	
Coarse balance, adjustable in 16 steps (polarity adjustable)	mV/V	± 0.08	
Fine balance, using screwdriver potentiometer	mV/V	± 0.08	
Measurement frequency range		Butterworth low-pass 3rd order, switchable	
at -1 dB	Hz	0...40	0...250
at -3 dB	Hz	50	300
Phase delay time	ms	7	1.1
Rise time	ms	10	1.6
Overshoot at sudden change in signal	%	<10	<10
Residual carrier voltage	%	<0.02	<0.2; typically 0.1
Input (symmetrical)			
Input impedance	$M\Omega$ par. pF	>10 470	
Permitted common-mode voltage	V	$\pm 6\text{ V}$	
Common-mode rejection	dB	0...600 Hz: >50	
Output (asymmetrical)			
Nominal voltage	V	± 10	
Permissible load resistance	$k\Omega$	>5	
Internal resistance	Ω	<5	
Noise , projected backwards to the input	$\mu\text{V/V}$	<0.2 (peak-to-peak); typically 0.1	<0.2 (peak-to-peak); typically 0.1
Linearity variance relative to nominal voltage	%	<0.02; typically 0.01	
Effect of temperature per 10 K in the nominal temperature range relative			
to sensitivity	%	<0.1; typically 0.05	
to the zero point at the amplifier output in the range 2 mV/V at $U_B=5\text{ V}$ ($4\times 350\ \Omega$) in the range 0.2 mV/V at $U_B=5\text{ V}$	mV mV	<4, or <13; also <0.05 % of the bridge balance value	
Long-term drift over 48 hours (after 1 h warm-up time)	$\mu\text{V/V}$	<0.05	

Connection boards

AP01



AP03




AP01 (connection board with D-connector)

Width	mm	20.3 (4 divs)
Transducer port		D-plug, 15-pin, DA-15P ¹⁾
Port for output signal		D-plug, 25-pin, DB-25P ²⁾
Option		2x EM001; 2x RM001 with AP02

AP03 (AP08 connection board with MS-connector)

Width	mm	40.6 (8 divs)
Transducer port		MS-cable plug, 7-pin, MS3106A 16S-1P ³⁾
Port for output signal		D-plug, 25-pin, DB-25P ²⁾
Option		2x EM001, 2x RM001 with AP02

AP11



AP11 (connection board with LEMO socket)

Width	mm	20.3 (4 divs)
Transducer port		LEMO FGG . 1B.306 6-pin ⁴⁾
Port for output signal		D-plug, 25-pin, DB-25P ²⁾
Option		2x EM001; 2xRM001 with AP02

1) HBM order number 2-9278.0321

2) HBM order number 2-9278.0293

3) HBM order number 1-MS3106PEMV

4) HBM order number 3-3312.0126

End phase module EM001

Input		
Input voltage	V	-10 ... +10
Input resistance	kOhm	12.5
Output		
Impressed voltage	V	-10 ... +10
Impressed current	mA	± 20 / 4 ... 20
Load resistance	Ohm	max. 500, min. 0
Measurement frequency range	kHz	0...10
Operating voltage	V	+16; -16
Current consumption	mA	35

Modifications reserved.

All details describe our products in general form only. They are not to be understood as express warranty and do not constitute any liability whatsoever.

B0603-2.4 en

Hottinger Baldwin Messtechnik GmbH

Im Tiefen See 45, D-64293 Darmstadt, Germany
Tel.: +49 6151 8030; Fax: +49 6151 803 9100
E-mail: support@hbm.com www.hbm.com



measurement with confidence